



**GeneQuery™ Human Neural Transmission and Membrane Trafficking  
 qPCR Array Kit  
 (GQH-NTM)  
 Catalog #GK008**

**Product Description**

ScienCell's GeneQuery™ human neural transmission and membrane trafficking qPCR array kit (GQH-NTM) is designed to facilitate gene expression profiling of key genes involved in (i) human neurotransmission; (ii) membrane trafficking; and (iii) related diseases such as generalized anxiety disorder, DDC deficiency, TH deficiency, and SPR deficiency. 88 genes are selected in this kit based on public database and literature research.

GeneQuery™ qPCR array kits are qPCR ready in a 96-well plate format, with each well containing one primer set that can specifically recognize and efficiently amplify a target gene's cDNA. The carefully designed primers ensure that: (i) the optimal annealing temperature in qPCR analysis is 65°C (with 2 mM Mg<sup>2+</sup>, and no DMSO); (ii) the primer set recognizes all known transcript variants of target gene, unless otherwise indicated; and (iii) only one gene is amplified. Each primer set has been validated by qPCR with melt curve analysis, and gel electrophoresis.

**GeneQuery™ qPCR Array Kit Controls**

Each GeneQuery™ plate contains eight controls (Figure 1).

- Five target housekeeping genes (β-actin, GAPDH, LDHA, NONO, and PPIH), which enable normalization of data.
- The Genomic DNA (gDNA) Control (GDC) detects possible gDNA contamination in the cDNA samples. It contains a primer set targeting a non-transcribed region of the genome.
- Positive PCR Control (PPC) tests whether samples contain inhibitors or other factors that may negatively affect gene expression results. The PPC consists of a predispensed synthetic DNA template and a primer set that can amplify it. The sequence of the DNA template is not present in the human genome, and thus tests the efficiency of the polymerase chain reaction itself.
- The No Template Control (NTC) is strongly recommended, and can be used to monitor the DNA contamination introduced during the workflow such as reagents, tips, and the lab bench.

**Kit Components**

Component	Quantity	Storage
GeneQuery™ array plate with lyophilized primers	1	4°C or -20°C
Optical PCR plate seal	1	RT
Nuclease-free H <sub>2</sub> O	2 mL	4°C

**Additional Materials Required (Materials Not Included in Kit)**

Component	Recommended

Reverse transcriptase	MultiScribe Reverse Transcriptase (Life Tech, Cat. #4311235)
cDNA template	Customers' samples
qPCR master mix	FastStart Essential DNA Green Master (Roche, Cat. # 06402712001)

### **Quality Control**

All the primer sets are validated by qPCR with melt curve analysis. The PCR products are analyzed by gel electrophoresis. Single band amplification is confirmed for each set of primers.

### **Product Use**

GQH-NTM is for research use only. It is not approved for human or animal use, or for application in clinical or *in vitro* diagnostic procedures.

### **Shipping and Storage**

The product is shipped at ambient temperature. Upon receipt, the plate should be stored at 4°C and is good for up to 12 months. For long-term storage (>1 year), store the plate at -20°C in a manual defrost freezer.

## Procedures

---

**Note:** The primers in each well are lyophilized.

1. Prior to use, allow plates to warm to room temperature.
2. Briefly centrifuge at 1,500x g for 1 minute before slowly peeling off the seal.
3. Prepare 20  $\mu$ l PCR reactions for one well as shown in Table 1.

Table 1

<b>cDNA template</b>	<b>0.2 – 250 ng</b>
2x qPCR master mix	10 $\mu$ l
Nuclease-free H <sub>2</sub> O	variable
<i>Total volume</i>	<i>20 <math>\mu</math>l</i>

**Important:** *Only use polymerases with hot-start capability to prevent possible primer-dimer formation. Only use nuclease-free reagents in PCR amplification.*

4. Add the mixture of 2x qPCR master mix, cDNA template, and nuclease-free H<sub>2</sub>O to each well containing the lyophilized primers. Seal the plate with the provided optical PCR plate seal.

**Important:** *In NTC control well, do NOT add cDNA template. Add 2x qPCR master mix and nuclease-free H<sub>2</sub>O only.*

5. Briefly centrifuge the plates at 1,500x g for 1 minute at room temperature. For maximum reliability, replicates are strongly recommended (minimum of 3).
6. For PCR program setup, please refer to the instructions of the master mix of the user's choice. We recommend a typical 3-step qPCR protocol for a 200nt amplicon:

### Three-step cycling protocol

Step	Temperature	Time	Number of cycles
Initial denaturation	95°C	10 min	1
Denaturation	95°C	20 sec	40
Annealing	65°C	20 sec	
Extension	72°C	20 sec	
Data acquisition	Plate read		
<i>Recommended</i>	<i>Melting curve analysis</i>		1
Hold	4°C	Indefinite	1

7. (Optional) Load the PCR products on 1.5% agarose gel and perform electrophoresis to confirm the single band amplification in each well.

Figure 1. Layout of GeneQuery™ qPCR array kit controls.

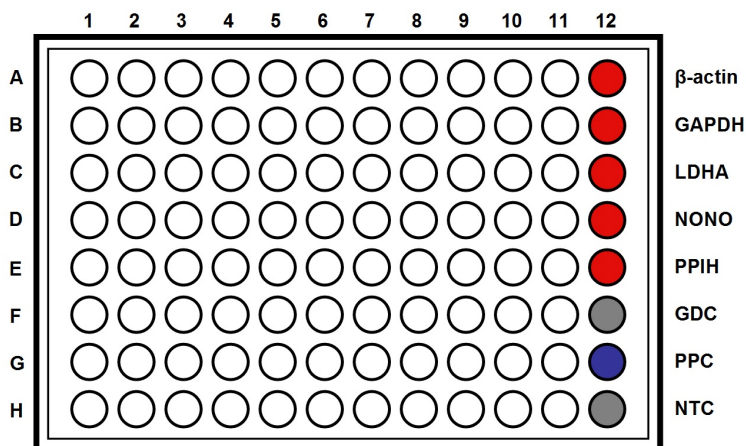



Table 2. Interpretation of control results:

<i>Controls</i>	<i>Results</i>	<i>Interpretation</i>	<i>Suggestions</i>
Housekeeping gene controls	Variability of a housekeeping gene's Cq value	The expression of the housekeeping gene is variable in samples; cycling program is incorrect	Choose a constantly expressed target, or analyze expression levels of multiple housekeeping genes; use correct cycling program and make sure that all cycle parameters have been correctly entered
gDNA Control (GDC)	Cq $\geq$ 35	No gDNA detected	N/A
	Cq < 35	The sample is contaminated with gDNA	Perform DNase digestion during RNA purification step
Positive PCR Control (PPC)	Cq > 30; or The Cq variations > 2 between qPCR Arrays.	Poor PCR performance; possible PCR inhibitor in reactions; cycling program incorrect	Eliminate inhibitor by purifying samples; use correct cycling program and make sure that all cycle parameters have been correctly entered
No Template Control (NTC)	Positive	DNA contamination in workflow	Eliminate sources of DNA contamination (reagents, plastics, etc.)

Figure 2. A typical amplification curve showing the amplification of a qPCR product.



Figure 3. A typical melting peak of a qPCR product.

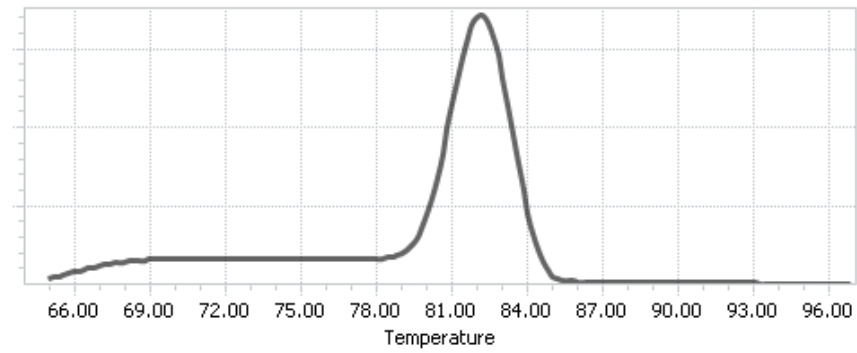



**GeneQuery™ Human Neural Transmission and Membrane Trafficking qPCR Array Kit  
(GQH-NTM)  
Catalog #GK008**

GeneQuery™ Human Neural Transmission and Membrane Trafficking qPCR Array Plate Layout\* (*8 controls* in Bold and Italic)

	<b>1</b>	<b>2</b>	<b>3</b>	<b>4</b>	<b>5</b>	<b>6</b>	<b>7</b>	<b>8</b>	<b>9</b>	<b>10</b>	<b>11</b>	<b>12</b>
<b>A</b>	ADRA1A	BDNF	CHRNA5	DRD2	GABRA2	GABRG3	GRIK1	GRM3	HTR2A	OPTN	SNAP25	<i><b>β-actin</b></i>
<b>B</b>	ADRA1D	BTD	CHRNA6	DRD4	GABRA4	GABRQ	GRIK2	GRM4	HTR2C	OTC	SOD1	<i><b>GAPDH</b></i>
<b>C</b>	ADRA2A	CHMP2B	CHRNA7	DRD5	GABRA5	GABRR2	GRIK4	GRM6	HTR3A	PTS	SPR	<i><b>LDHA</b></i>
<b>D</b>	ADRB2	CHRM1	CHRNE	FIG4	GABRB1	GCH1	GRIK5	GRM7	HTR4	QDPR	TARDBP	<i><b>NONO</b></i>
<b>E</b>	ADRB3	CHRM4	COMT	FUS	GABRB3	GH1	GRIN2A	HTR1A	HTR7	RAB10	TH	<i><b>PPIH</b></i>
<b>F</b>	AKR1B1	CHRM5	DBH	G6PD	GABRE	GRIA1	GRIN2B	HTR1B	LLGL1	SLC6A2	TPH1	<i><b>GDC</b></i>
<b>G</b>	ALDH5A1	CHRNA3	DHFR	GABBR1	GABRG1	GRIA2	GRIN2C	HTR1D	LPL	SLC6A3	VAPB	<i><b>PPC</b></i>
<b>H</b>	ALS2	CHRNA4	DRD1	GABBR2	GABRG2	GRIA3	GRM1	HTR1F	MAOA	SLC6A4	VCP	<i><b>NTC</b></i>

\* gene selection may be updated based on new research and development